

# BD Insyte™, Insyte-W™, and Insyte-N™ IV Catheters



with BD Vialon™ Catheter Material

| BD Insyte™ IV Catheter |               |                  |                     |        |
|------------------------|---------------|------------------|---------------------|--------|
| Ref #                  | Gauge         | Length           | Flowrate (mL / min) | Color  |
| 381212                 | 24 G (0.7 mm) | 0.75 in. (19 mm) | 25                  | Yellow |
| 381223                 | 22 G (0.9 mm) | 1.00 in. (25 mm) | 35                  | Blue   |
| 381233                 | 20 G (1.1 mm) | 1.00 in. (25 mm) | 65                  | Pink   |
| 381234                 | 20 G (1.1 mm) | 1.16 in. (30 mm) | 60                  | Pink   |
| 381237                 | 20 G (1.1 mm) | 1.88 in. (48 mm) | 55                  | Pink   |
| 381244                 | 18 G (1.3 mm) | 1.16 in. (30 mm) | 105                 | Green  |
| 381247                 | 18 G (1.3 mm) | 1.88 in. (48 mm) | 95                  | Green  |
| 381254                 | 16 G (1.7 mm) | 1.16 in. (30 mm) | 220                 | Grey   |
| 381257                 | 16 G (1.7 mm) | 1.77 in. (45 mm) | 205                 | Grey   |
| 381267                 | 14 G (2.1 mm) | 1.75 in. (45 mm) | 330                 | Orange |

| BD Insyte-W™ IV Catheter with Wings |               |                  |                     |        |
|-------------------------------------|---------------|------------------|---------------------|--------|
| Ref #                               | Gauge         | Length           | Flowrate (mL / min) | Color  |
| 381312                              | 24 G (0.7 mm) | 0.75 in. (19 mm) | 25                  | Yellow |
| 381323                              | 22 G (0.9 mm) | 1.00 in. (25 mm) | 35                  | Blue   |
| 381333                              | 20 G (1.1 mm) | 1.00 in. (25 mm) | 65                  | Pink   |
| 381334                              | 20 G (1.1 mm) | 1.16 in. (30 mm) | 60                  | Pink   |
| 381337                              | 20 G (1.1 mm) | 1.88 in. (48 mm) | 55                  | Pink   |
| 381344                              | 18 G (1.3 mm) | 1.16 in. (30 mm) | 105                 | Green  |
| 381347                              | 18 G (1.3 mm) | 1.88 in. (48 mm) | 95                  | Green  |
| 381354                              | 16 G (1.7 mm) | 1.16 in. (30 mm) | 220                 | Grey   |
| 381357                              | 16 G (1.7 mm) | 1.77 in. (45 mm) | 205                 | Grey   |

| BD Insyte-N™ IV Catheter |               |                  |                     |        |
|--------------------------|---------------|------------------|---------------------|--------|
| Ref #                    | Gauge         | Length           | Flowrate (mL / min) | Color  |
| 381211                   | 24 G (0.7 mm) | 0.56 in. (14 mm) | 25                  | Yellow |
| 381311 (Winged)          | 24 G (0.7 mm) | 0.56 in. (14 mm) | 25                  | Yellow |

Shipping cases contain 200 units (4 boxes of 50)

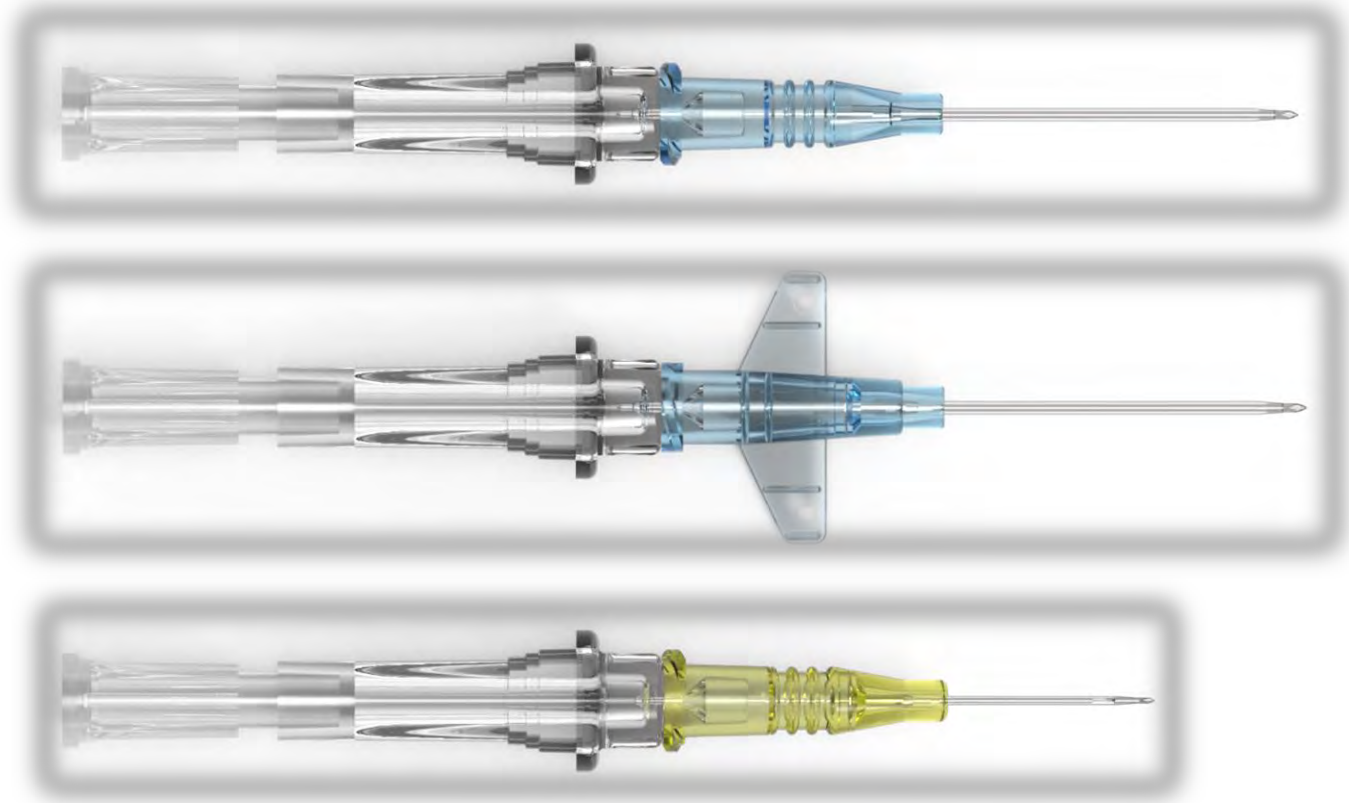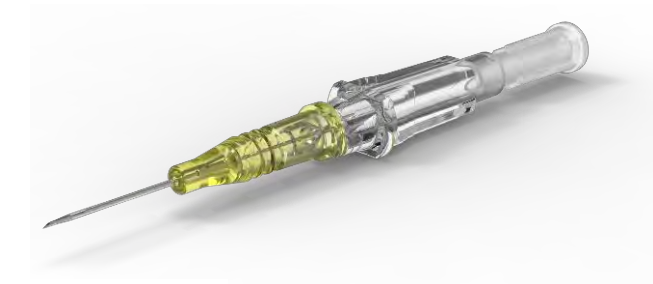

35 years of excellence, billions sold globally

bd.com

BD, the BD Logo, Instaflash, Insyte, Insyte-N, Insyte-W and Vialon are trademarks of Becton, Dickinson and Company or its affiliates. © 2020 BD. BD-18048 (06/20)



BD Insyte™ IV Catheter

Non-ported, straight IV catheter with BD Vialon™ Catheter Material

Radiopaque **BD Vialon™ Catheter Material**


18-22 G devices support **power injection at 300 psi**

**Sharp needle and tapered catheter tip** allow for a smooth, easy insertion

**Transparent catheter hub** offers clear visibility of blood flashback

**Non-ported** design may reduce chances of mechanical and infectious complications<sup>1</sup>

Not made with **latex, DEHP, or BPA**

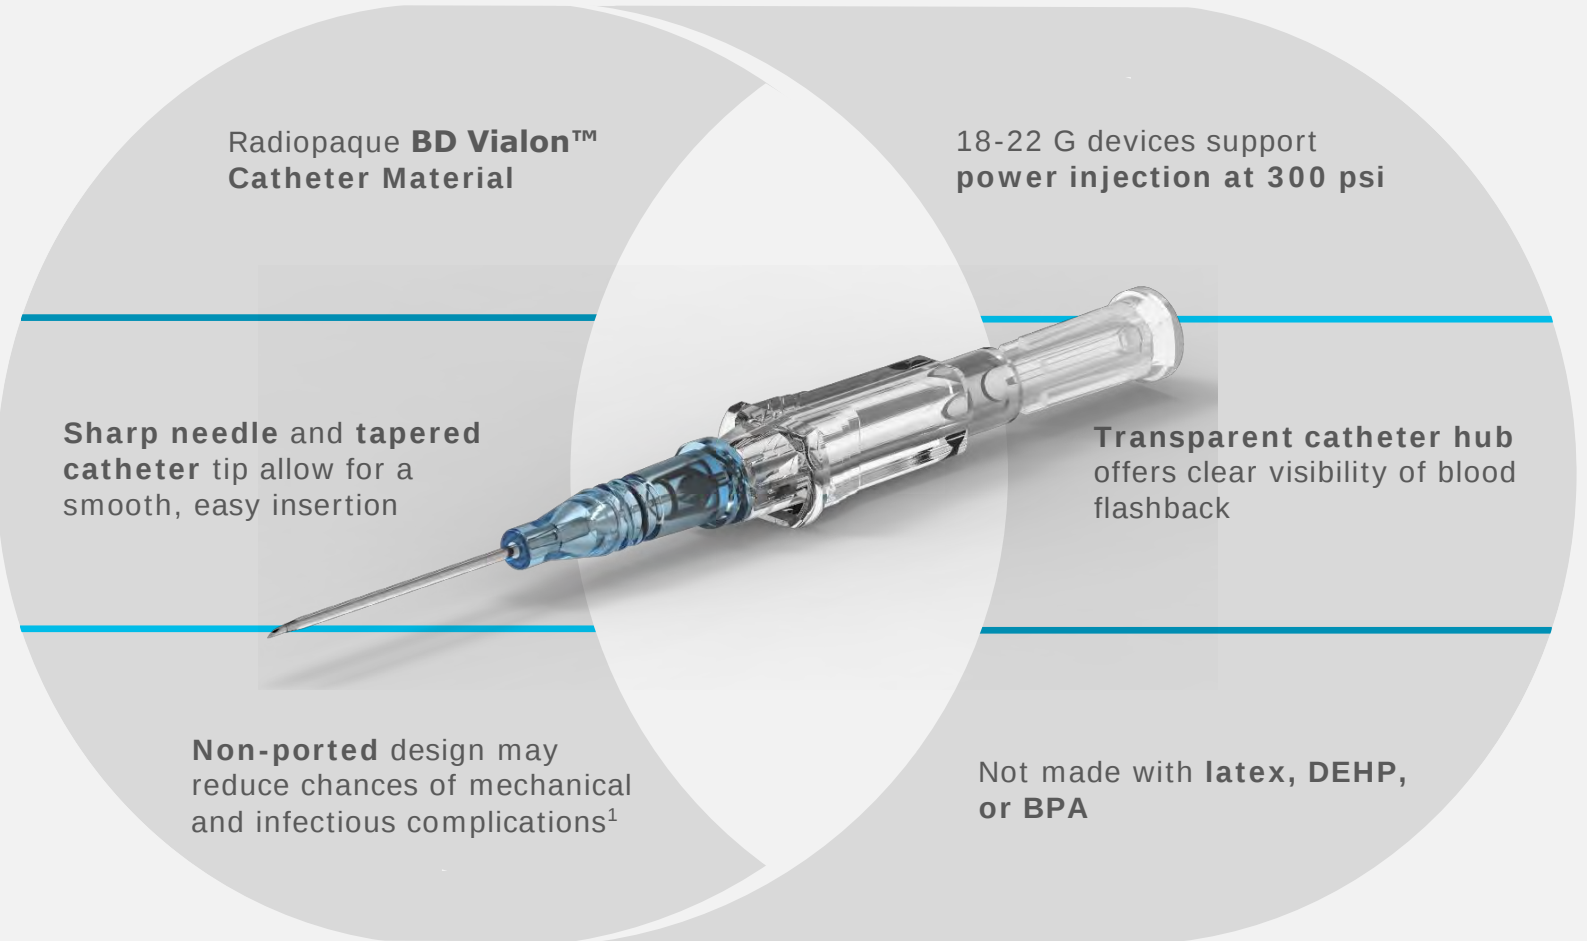




The BD Vialon™ Catheter Material Difference

**More than 15 clinical studies** conducted over 25 years have demonstrated that IV catheters made of BD Vialon™ Catheter Material demonstrated **easier to insert** or provide **longer dwell times** compared to FEP catheters.<sup>2-17</sup>

Improved patient comfort

Proprietary BD Vialon™ Catheter Material **softens up to 70 % in the vein.**

BD Vialon™ Catheter Material has **greater kink resistance than FEP.**<sup>2</sup>

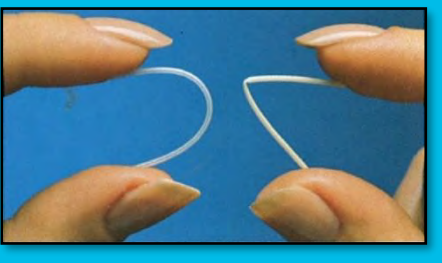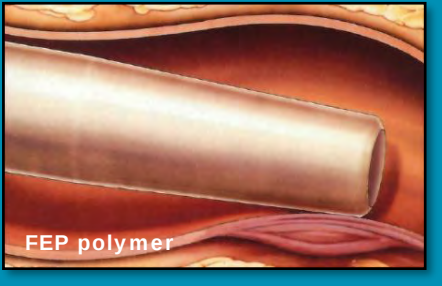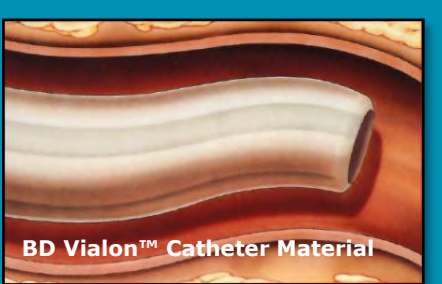


Reduced complications

BD Vialon™ Catheter Material **reduces the chance of mechanical phlebitis** by up to 50% compared to FEP.<sup>3</sup>

“On average, Vialon remained in situ for **9 additional hours** or 21% longer than Teflon before infiltrating.”<sup>4</sup>

BD Insyte-W™ IV Catheter with Wings


All the benefits of BD Insyte™ IV Catheter with the **added benefits of wings**

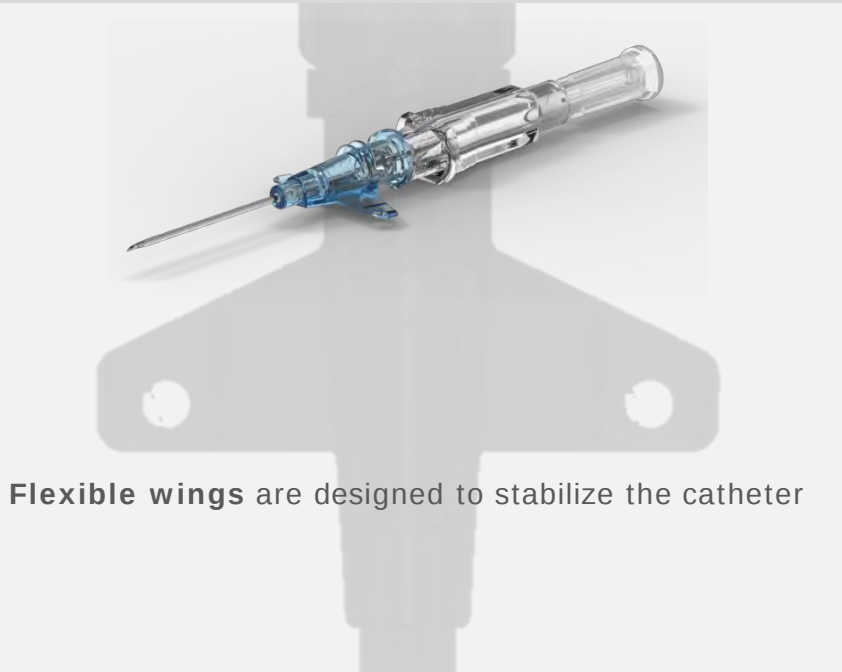

**Flexible wings** are designed to stabilize the catheter

BD Insyte-N™ IV Catheter

Designed to accommodate **smaller veins**

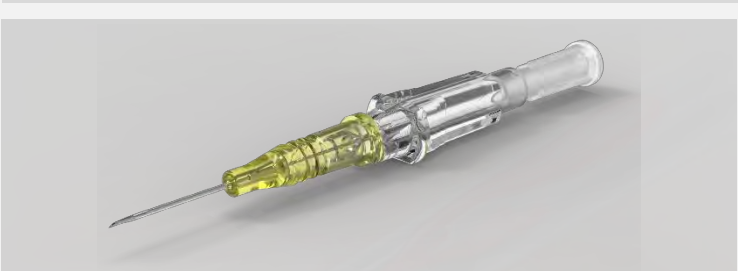

**Small gauge**  
(24 G / 0.7 mm)

**Short length**  
(0.56 in. / 14 mm)

**BD Instaflash™ Needle Technology** incorporates a notched needle, which is designed to confirm immediate vessel entry, improve first-stick success, and reduce painful hit-and-miss insertions

References

1. Dougherty L, Lister SE. The Royal Marsden Hospital Manual of Clinical Nursing Procedures. 9th ed. Malden, MA: Wiley Blackwell Publishing; 2015.
2. Gaukroger PB, Roberts JG, Manners TA. Infusion thrombophlebitis: a prospective comparison of 645 Vialon and Teflon cannulae in anaesthetic and postoperative use. *Anaesthesia and Intensive Care*. 1988; 16:265-271.
3. Maki DG, Ringer M. Risk factors for infusion-related phlebitis with small peripheral venous catheters. *Annals of Internal Medicine*. 1991; 114:845-854.
4. Stanley MD, Meister E, Fuschuber K. Infiltration during intravenous therapy in neonates: comparison of Teflon® and Vialon® catheters. *Southern Medical Journal*. 1992; 85:883-886.
5. Jacquot C, Fauvage B, Bru JP, Croize J, Calop J. Effect of type of material on thrombophlebitis risk with peripheral venous catheters. *Ann Fr Anestha Réanim*. 1989; 8:3-7. [French language]
6. Fassolt A. Phlebitogenicity of venous catheters of Vialon. *Infusionsther Klin Ernahr*. 1985;12(6):282-2866.
7. Foster L, Wallis M, Paterson B, James H. A descriptive study of peripheral intravenous catheters in patients admitted to a pediatric unit in one Australian hospital. *J Infus Nurs*. 2002;23(3):159-167.
8. Karadag A, Gorgulu S. Effect of two different short peripheral catheter materials on phlebitis development. *J Infus Nurs*. 2003;23(3):158-166.
9. Kerrison T, Woodhull J. Reducing the risk of thrombophlebitis. Comparison of Teflon and Vialon cannulae. *Professional Nurse*. 1994;9(10):662-666.
10. Lai KK. Safety of prolonging peripheral cannula and IV tubing use from 72 hours to 96 hours. *AJIC*. 1998;25(1):66-70.
11. McKee JM, Shell JA, Warren TA, Campbell VP. Complications of intravenous therapy: a randomized prospective study—Vialon vs. Teflon. *J Infus Nurs*. 1989;12(5):288-295.
12. Myles PS, Buckland MR, Burnett WJ. Single versus double occlusive dressing technique to minimize infusion thrombophlebitis: Vialon® and Teflon® cannulae reassessed. *Anaesth Intens Care*. 1991; 19:525-529.
13. Stoddard GJ, Davis HT. Development of thrombophlebitis in peripheral veins with Vialon and PTFE-Teflon cannulas: a double-blind, randomised, controlled trial. *Ann R Coll Surg Engl*. 1993; 74:296-299.
14. Shotkin JD, Lombardo F. Use of an indwelling peripheral catheter for 3-5 day chemotherapy administration in the outpatient setting. *J Infus Nurs*. 1996;19(6):315-320.
15. Stonehouse J, Butcher J. Phlebitis associated with peripheral cannulae. *Professional Nurse*. 1996;12(1):51-54.
16. Szycher M. Biostability of polyurethane elastomers: a critical review. *J Biomaterial Applications*. 1998; 3:297-402.
17. Treuren BC, Galletly DC. A comparison of intravenous cannulae available in New Zealand. *Anaesth Intens Care*. 1990;18(4):540-546.